

INTERNATIONAL STANDARD

ISO
10079-1

First edition
1991-05-15

Medical suction equipment —

Part 1:

**Electrically powered suction equipment — Safety
requirements**

Matériel d'aspiration médical —

Partie 1: Matériel électrique d'aspiration — Prescriptions de sécurité



Reference number
ISO 10079-1 : 1991 (E)

Contents

	Page
Section 1: General	
1.1 Scope	1
1.2 Normative references	2
1.3 Definitions	3
1.4 General requirements and general requirements for tests	4
1.5 Classification	4
1.6 Identification, marking and documents	4
1.7 Power input	5
Section 2: Environmental conditions	
2.8 Basic safety categories	6
2.9 Removable protective means	6
2.10 Environmental conditions	6
2.11 Special measures with respect to safety	6
2.12 Single fault condition	6
Section 3: Protection against electric shock hazards	
3.13 General	7
3.14 Requirements related to classification	7
3.15 Limitation of voltage and/or energy	7
3.16 Enclosures and protective covers	7
3.17 Separation	7

3.18	Protective earthing, functional earthing and potential equalization	7
3.19	Continuous leakage currents and patient auxiliary currents	7
3.20	Dielectric strength	7
Section 4: Protection against mechanical hazards		
4.21	Mechanical strength	8
4.22	Moving parts	8
4.23	Surfaces, corners and edges	8
4.24	Stability in normal use	8
4.25	Expelled parts	8
4.26	Vibration and noise	8
4.27	Pneumatic and hydraulic power	8
4.28	Suspended masses	8
Section 5: Protection against hazards from unwanted or excessive radiation		
5.29	X-radiation	9
5.30	Alpha, beta, gamma, neutron radiation and other particle radiation	9
5.31	Microwave radiation	9
5.32	Light radiation (including lasers)	9
5.33	Infra-red radiation	9
5.34	Ultraviolet radiation	9
5.35	Acoustical energy (including ultra-sonics)	9
5.36	Electromagnetic compatibility	9
Section 6: Protection against hazards of ignition of flammable anaesthetic mixtures		
6.37	Locations and basic requirements	10
6.38	Marking and accompanying documents	10
6.39	Common requirements for AP and APG equipment	10
6.40	Requirements and tests for AP equipment, parts or components	10
6.41	Requirements and tests for APG equipment, equipment parts or components	10
Section 7: Protection against excessive temperatures and other safety hazards		
7.42	Excessive temperatures	11
7.43	Fire prevention	11
7.44	Overflow, spillage, leakage, humidity, ingress of liquids, cleaning, sterilization and disinfection	11

7.45	Pressure vessels and parts subject to pressure	13
7.46	Human errors	13
7.47	Electrostatic charges	13
7.48	Materials in applied parts in contact with body of patient	13
7.49	Interruption of power supply	13

Section 8: Accuracy of operating data and protection against hazardous output

8.50	Accuracy of operating data	14
8.51	Protection against hazardous output	14

Section 9: Abnormal operation and fault conditions: environmental tests

9.52	Abnormal operation and fault conditions	15
9.53	Environmental tests	15

Section 10: Constructional requirements

10.54	General	16
10.55	Enclosures and covers	16
10.56	Components and general assembly	16
10.57	Mains parts, components and layout	18
10.58	Protective earth terminals	18
10.59	Construction and layout	18

Figures

1	Schematic drawing illustrating suction equipment	2
2	Typical test apparatus for evaluating leakage of collection container for general use	12
3	Typical test apparatus for evaluating leakage of collection container designated for use in thoracic drainage system	12
4	Typical test apparatus for evaluating thoracic drainage system performance	16
5	Test apparatus for suction tubing tests	18
6	Test apparatus for thoracic drainage	19
7	Test apparatus for battery-powered transportable suction equipment	20
8	Apparatus for testing resistance to implosion of collection container	21

Annexes

M	Rationale statement	22
N	Table of typical range of volumes for collection containers for specific uses	23
P	Lumen (passageway) size and its effects on flow	24

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 10079-1 was prepared by Technical Committee ISO/TC 121, *Anaesthetic and respiratory equipment*, Sub-Committee SC 8, *Suction devices for hospital and emergency care use*.

ISO 10079 consists of the following parts, under the general title *Medical suction equipment*:

- *Part 1: Electrically powered suction equipment — Safety requirements*
- *Part 2: Non-electrical manually powered suction equipment*
- *Part 3: Non-electrical suction equipment powered from a vacuum or pressure source*

Annexes M, N and P of this part of ISO 10079 are for information only.

Introduction

This part of ISO 10079, which has been prepared under the responsibility of Sub-Committee 8 of ISO/TC 121, comprises Part 1 of the standard for Medical Suction Equipment, and deals only with safety requirements for electrically powered suction equipment.

Suction is used to clear the airway and remove unwanted material from body cavities. Suction is also used to assist drainage and decompress body cavities. Suction and vacuum systems are used widely both in health care facilities such as hospitals, for domiciliary care of patients who are nursed at home, and in emergency situations both outside hospitals in field conditions, and during transport in ambulances.

In this part of ISO 10079, vacuum readings are specified as gauge (relative) pressures to assist clinical personnel. However, this is not intended to prevent engineering groups from using absolute vacuum in their design process.

Test methods other than those specified in this part of ISO 10079, but of equal or greater accuracy, may be used to verify compliance with the given requirements. However, in the event of a dispute, the methods specified in this part of ISO 10079 are to be used as the reference methods.

A rationale for the most important requirements is given in annex M. It is considered that a knowledge of the reasons for the requirements will not only facilitate the proper application of the standard, but will expedite any subsequent revision. This annex does not form part of the standard.

Medical suction equipment —

Part 1:

Electrically powered suction equipment — Safety requirements

Section 1: General

1.1 Scope

NOTE — See also annex M (in this part of ISO 10079).

ISO 10079-1 is one of a series of International Standards based on IEC 601-1; in IEC 601-1 (the “General Standard”), this type of International Standard is referred to as a “Particular Standard”. As stated in 1.3 of IEC 601-1 : 1988, the requirements of this International Standard take precedence over those of IEC 601-1.

The Scope and Object given in clause 1 of IEC 601-1 : 1988 applies except that 1.1 shall be replaced by the following:

This part of ISO 10079 specifies minimum safety and performance requirements for medical and surgical suction equipment (see figure 1) in health care facilities such as hospitals, for domiciliary care of patients and for field and transport use. Although equipment may be driven by centrally powered piped vacuum systems, compressed gases, electricity or be manually powered for a variety of applications, this part addresses only equipment powered electrically.

Excluded from the standard are:

- a) central power supply (by vacuum/compressed air generation), piping systems of vehicles and buildings, and wall connectors;


- b) catheter tubes, drains, curettes and suction tips;
- c) syringes;
- d) dental suction equipment;
- e) waste gas scavenging systems;
- f) laboratory suction;
- g) autotransfusion systems;
- h) passive urinary drainage;
- i) closed system for wound drainage;
- j) gravity gastric drainage;
- k) orally operated mucous extractors;
- l) suction equipment where the collection container is downstream of the vacuum pump;
- m) equipment marked as suction unit for permanent tracheostomy;
- n) ventouse (obstetric) equipment;
- o) neonatal mucous extractors;
- p) suction equipment marked for endoscopic use only.

Applicable standard:

Electrically powered
suction equipment
(ISO 10079-1)

Non-electrical manually
powered suction equipment
(ISO 10079-2)

Non-electrical equipment
powered from a vacuum or
pressure source
(ISO 10079-3)

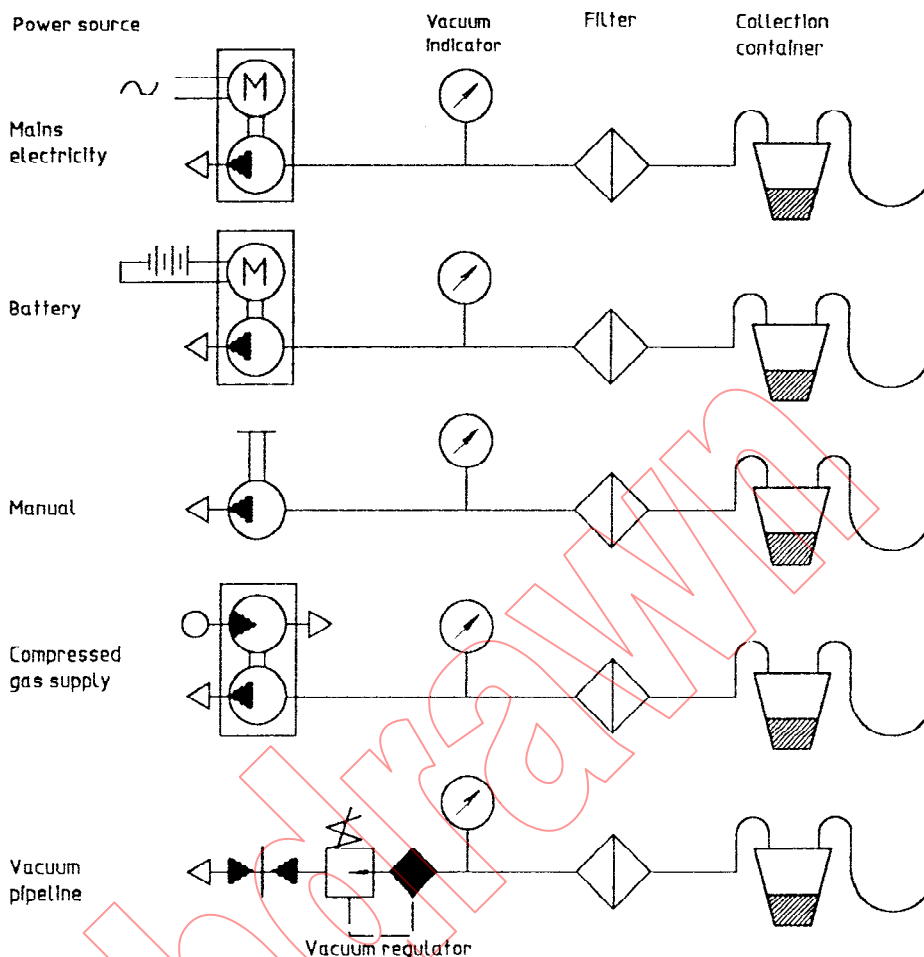

NOTES

- 1 This part of ISO 10079 applies to mains electricity and battery-powered suction equipment.
Part 2 of ISO 10079 applies to non electrical manually powered suction equipment.
Part 3 of ISO 10079 applies to non-electrical suction equipment powered from a vacuum or pressure source.
- 2 Components illustrated are not necessarily required by this International Standard.
- 3 Suction equipment shown are only examples, and actual systems may consist of other arrangements and components not illustrated in the figure.

Figure 1 — Schematic drawing illustrating suction equipment

1.4 Environmental conditions

The requirements given in 1.4 of IEC 601-1 apply except that the following modification shall be made to 1.4 b) 1).

Substitute “+ 5 °C” for “+ 10 °C” and “+ 35 °C” for “40 °C”.

For field and transport use, environmental conditions shall be as specified in 53.

1.2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this part of ISO 10079. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to

agreements based on this part of ISO 10079 are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 32: 1977, *Gas cylinders for medical use — Marking for identification of content*.

ISO 3743: 1988, *Acoustics — Determination of sound power levels of noise sources — Engineering methods for special reverberation test rooms*.

ISO 3744: 1981, *Acoustics — Determination of sound power levels of noise sources — Engineering methods for free-field conditions over a reflecting plane*.

ISO 5356-1: 1987, *Anaesthetic and respiratory equipment — Conical connectors — Part 1: Cones and sockets*.

IEC 529 : 1976, *Classification of degrees of protection provided by enclosures.*

IEC 601-1 : 1988, *Medical electrical equipment — Part 1: General requirements for safety.*

IEC 651 : 1979, *Sound level meters.*

IEC 695-2-2 : 1980, *Fire hazard testing — Part 2: Test methods — Needle-flame test.*